
www.hidenanalytical.com info@hiden.co.uk



# **Hiden QIC BioStream**

### For fermentation off-gas analysis







### Introduction

- This presentation provides an overview of gas analysis systems for fermentation off gas analysis.
- Fermentation off gas analysis by mass spectrometry provides real time trend analysis of the gases and vapour species that are important to product yield, O<sub>2</sub> CO<sub>2</sub> H<sub>2</sub> CH<sub>4</sub> for example, and provides vital data for real time process monitoring.
- The mass spectrometer is user programmable to analyse a broad range of gas and vapour species and covers most species of interest in both aerobic and anaerobic applications.
- The QIC series gas analysers manufactured by Hiden Analytical include systems configured to address the application of fermentation off gas analysis.



### Hiden QIC Series Gas Analysis Systems

• The QIC series gas analysers are mass spectrometers configured for real time gas analysis, fermentation off gas for example.

•The QIC systems provide for multiple species real time trend analysis providing quantitative gas analysis.


•The QIC systems include an inert silica capillary with fast response to both gases and vapours.



QGA A single stream real time gas analyser




# **QIC Inlet Technology**

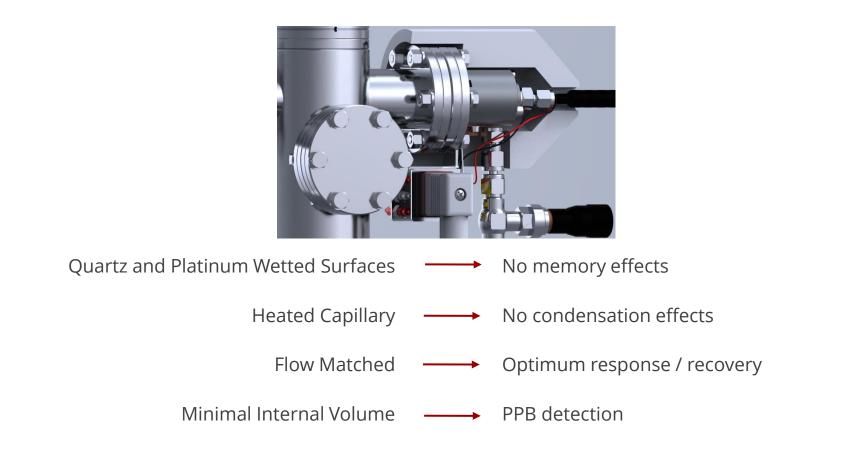



### These features provide excellent analyser performance for fermentation off-gas analysis



### **QIC Inlet- MS Interface Overview**



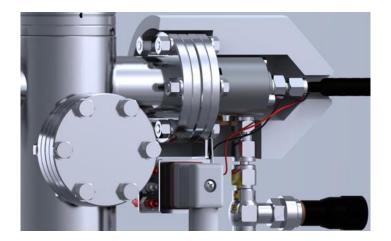

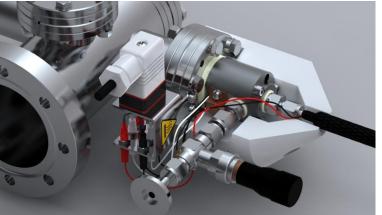


Key G1 Penning gauge VR1 QIC Inlet bypass control valve P1 60 I/s turbo drag pump P2 Backing and bypass Scroll pump MS UHV Housing (Mass spectrometer chamber)

info@hiden.co.uk



### Fast Response to Permanent Gases / Vapours

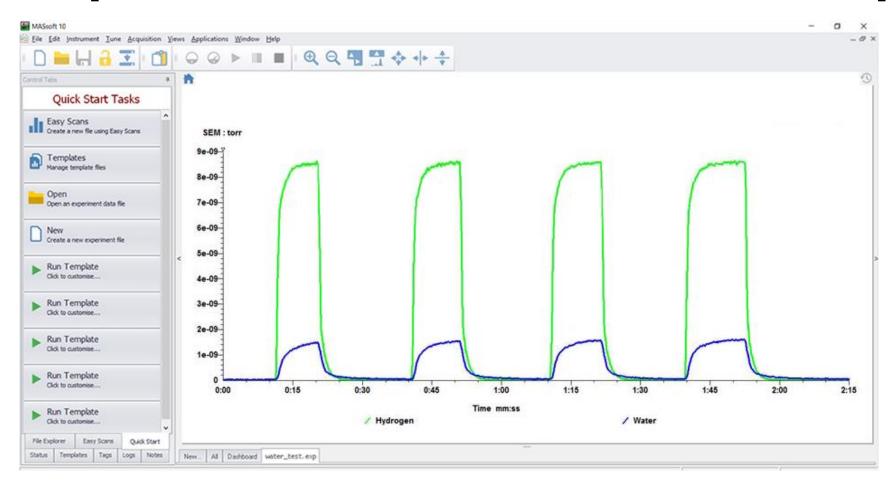

Data shows the response of the QIC inlet to gas and vapour during switching between a dry He stream and a wet  $H_2$  and Ar flow. For clarity, only the  $H_2$  and  $H_2O$  data is shown in the graph.



### **QIC BioStream**

Modular multi-stream off-gas analyser, bench top or cart configured for analysis of:


8, 20, 40 or 80 sample streams for:

• high flow ~ up to 12 l/min sample flow

#### Or

- 20, 40 or 80 sample streams for:
- low flow small volume reactors 4 ml/min sample flow

For flow rates up to 12 l/minute the QIC BioStream can measure selected stream flow rate. For higher flow rates, sample flow is connected to the QIC BioStream via a T piece.







### QIC BioStream-C bench top system

Modular configuration:

Small footprint instrument: 535mm deep X 530mm wide

20 stream version shown with dual mass flow meters for accurate selected flow measurement in the flow range to 12 l/min.






### QIC BioStream-C bench top system

Small footprint instrument: 535mm deep X 530mm wide


Top mounted Proteus Valve 20, or 40 stream versions.

20 stream version shown with dual mass flow meters for accurate selected flow measurement in the flow range to 12 l/min.

Flow measurement is for the  $O_2$  uptake (OUR) and  $CO_2$  expiration rate (CER) calculations.

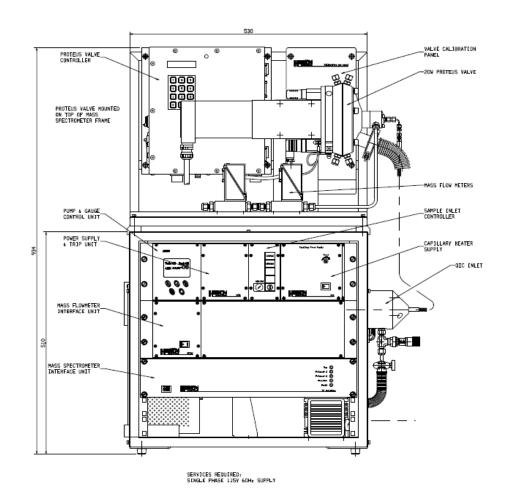




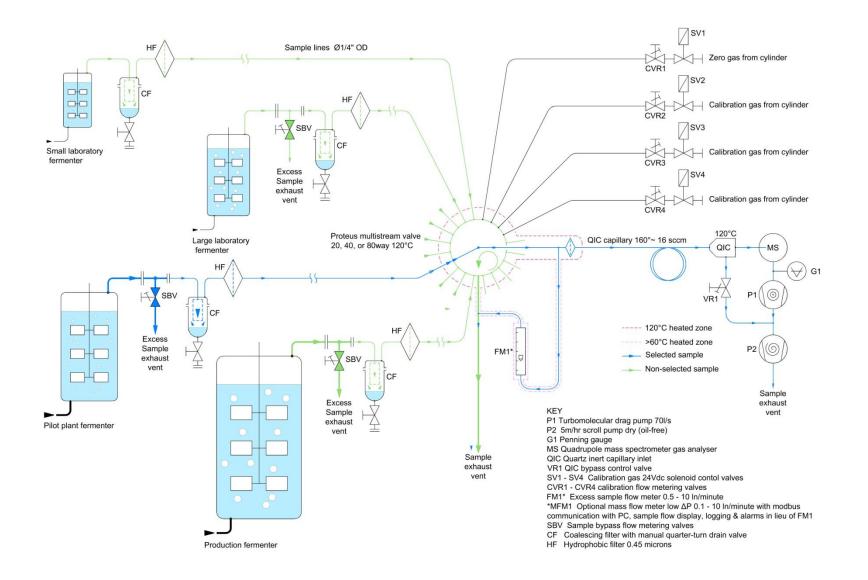



### QIC BioStream switching time between sample streams in > 0.6 seconds

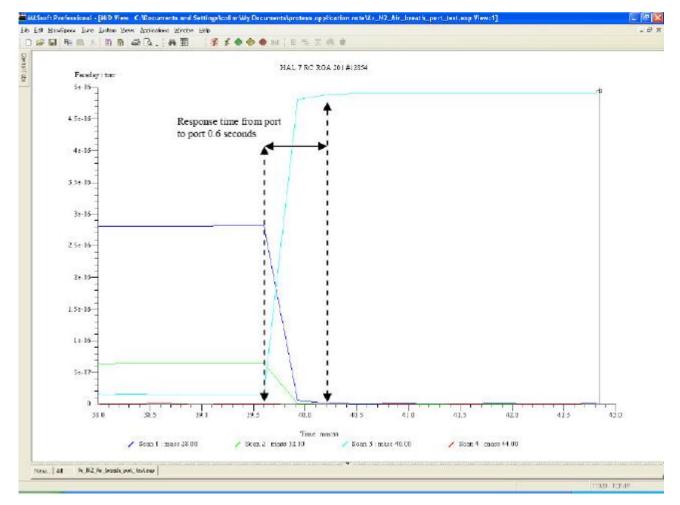


www.HidenAnalytical.com





<u>Hiden I</u>	Proteus Multistream Valve
Туре	Gas Selector valve - relies on novel face sealing technology to provide effective sealing with long life.
Max Operating Temperature	120°C
Minimum Sample Flow	Not applicable - Determined by analyser (no sample lost)
'Crosstalk' from other samples	Zero
Number of operations before maintenance	>6 x 106
Memory (carry over) From previous sample	Class leading low memory due to minimised internal switching volume and low sample wetted surface area. The face seal is isolated from the sample by a secondary internal seal.
Number of ports	20, 40, 80
Actuation	Direct drive, high torque microstepping motor with IP65 protected incremental rotary encoder providing home z-position and closed loop motion control. Full motion management including intelligent acceleration/deceleration, position maintenance, bi-directional drive and position error annunciation.

Positioning accuracy	+/- 0,09°
	Vac
Full brown-out sensing and protection	Yes
Communication (valve port position select)	Binary, BCD RS232C
Available as separate product	Yes

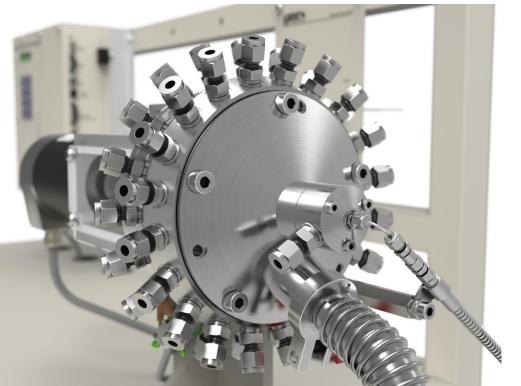





### **Triple Filter Quadrupole Mass Spectrometer**

- Precision machined ceramic supports
- Independently driven RF pre and post filters
- Long term stable operation

1.4769

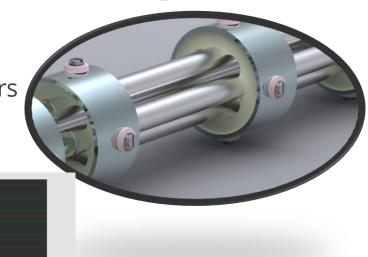


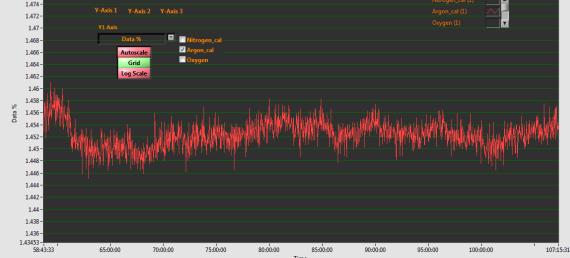

- Oxygen, Nitrogen and Argon measured over 110 hours
- Data shows stability of the Argon signal for an extended period



### QGA 2 Software for Quantitative Gas Analysis

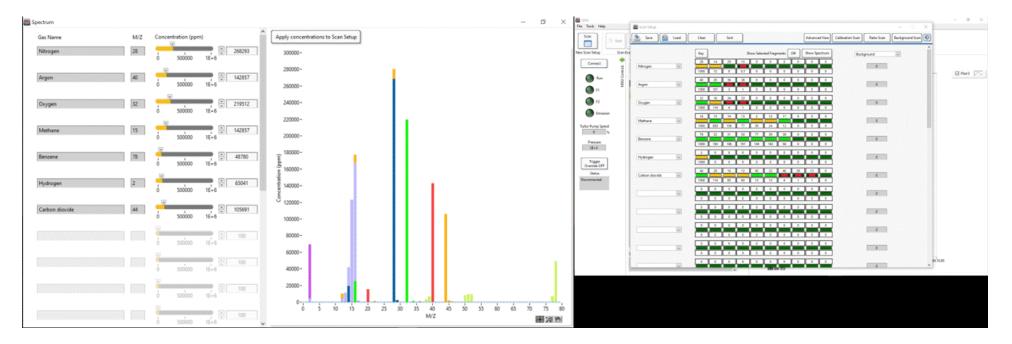


An application specific software package for quantitative gas and vapour analysis providing real time continuous analysis of up to 32 species with concentrations measured in the range 5PPB to 100%

- Automatic subtraction of spectral overlaps
- Automated calibration routines
- Mass spectral library with intelligent scan feature
- Multi-stream support




# Multiple stream sequence set up - 80 stream example

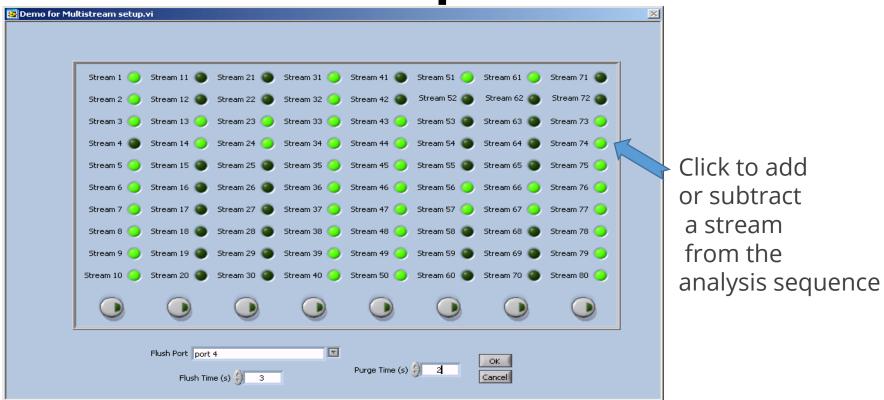

Fermenters can be added or subtracted from the stream sequence at any time during the analysis with a simple click on the stream LED.



### Multi stream gas analysis - The real time trend analysis of up to 4 selected streams can be viewed in real time and in review

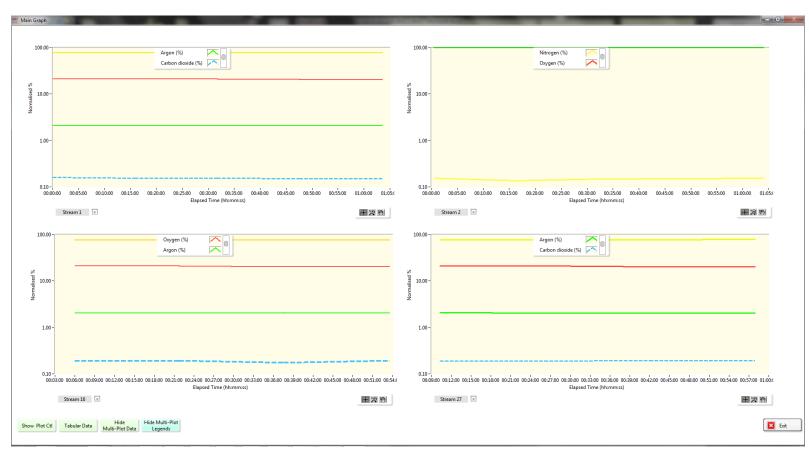

www.HidenAnalytical.com

#### Data Export

- Data export to MS Excel.
- New workbook for each data file.

9	Die Dat	yer poet	Fgrad Io	shi Data 198	ndow thelp										7/04	e a question for f	ielo 🔹 💶 i
1	🛯 🖬 🔒	0127	81. I X II	12.00	9.0.1	🤶 Σ 🔹	21 31 1 31	🦂 107% 🔹	ans Ans		* 10 ·	BI		i 🗟 🦉 %	· 58 d	日午日・	<u>0. A</u> -
a	2020	000	6 2 5	A YW Repl	with Changes	End Re	vien						_				
	At	* <u>6</u> M	tode = Mix	ture													
	A	B	C	0	E	F	G	н	1	J	K	L	M	N	0	Ρ	Q
í I	Mode - M	sture															
		fault Speed															
2																	
	experiment	r Start time: 1	0:15:54 0.4	te: 12 Feb 20	112												
4		Gas	CO	npo	sitio	n	E F	RAW	dat	а			0	orre	cted	d dat	a
4	0GA - 5	Gas	COI	mpo	sitio	n	Raw Dota	RAW					Corrected	orre			
4	OGA - % Time (ms)	Gas Nitrogen 28	CO Argen 40	npo Oxygen 32	Sitio Water 18	n	Time (ms)	Nitrogen 28	Argon 40	Oxygen 32			Time (ms)	Nitrogen 28	Argon 40	Oxygen 32	Water 18
4	0GA - 5	Gas	COI	0xygen 32 18.124	Sitio Water 18 0.714	n					Water 18 1.06E-09		Certected	Data		Oxygen 32	
4	OGA - % Time (ms)	Gas Nitrogen 28	CO Argen 40	npo Oxygen 32	Sitio Water 18	n	Time (ms)	Nitrogen 28	Argon 40	Oxygen 32			Time (ms)	Nitrogen 28	Argon 40	0xygen 32 2.82E-08	Water 18
4 5 7 8	OGA - 5 Time (ms) 5638	Gas Nitrogen 28 80.149	CO Argen 40 1.014	0xygen 32 18.124	Sitio Water 18 0.714	n	Time (ms) 5.64E+03	Nitrogen 28 1 27E-07	Argon 40 1.45E-09	0xygen 32 2.67E-08	1.06E-09		Time (ms) 5.64E+03	Nitrogen 28 1.25E-07	Argon 40 1.58E-09	0xygen 32 2.82E-08 2.81E-08	Water 18 1.11E-09
4 5 7	0GA - % Time (ms) 5638 36480	Gas Nitrogen 28 80.149 80.198	CO Argen 40 1.014 1.004	0xygen 32 18.124 18.094	Sitio Water 18 0.714 0.704	n	Time (ms) 5.64E-03 3.65E-04	Nitrogen 28 1 27E-07 1 26E-07	Argon 40 1.45E-09 1.43E-09	0xygen 32 2.67E-08 2.66E-08	1.06E-09 1.04E-09		Time (ms) 5.64E+03 3.65E+04	Nitrogen 28 1.25E-07 1.25E-07	Argon 40 1.58E-09 1.58E-09	0xygen 32 2.82E-08 2.81E-08 2.81E-08	Water 18 1.11E-09 1.09E-09

\_ 5 ×

Type a question for help 🔍 🗕 🖶 🗙

- Quantitative data, raw data values and corrected data values are exported.
- Calibration factors and background correction values are recorded.

IN	0	Р	Q	R	3		0
					09.Feb-09 Ca	libration	factor
gen 28	Argon 40	Oxygen 32	Water 18		Background	Calibration Fa	ctor
26E-07	1.58E-09	2.82E-08	1.11E-09		8.19E-11	1.01349	
25E-07	1.56E-09	2.81 E-08	1.09E-D9		1.58E-10	0.91654	
24E-07	1.55E-09	2.81 E-08	1.11E-09		1.54E-10	0.9474	
24E-07	1.55E-09	2.80E-08	1.09E-09		1.14E-09	0.95104	
24E-07	1.55E-09	2.79E-08	1.12E-D9		0	1	
24E-07	1.54E-09	2.82E-08	1.11E-09		0	1	
14E 0T	1 55 5 00	1 01 E N0	1.11E D2		0	1	

- 10 - B / U = = = = 3 🧐 % , % 🕮 🛱 🖽 - 加 - 🗛 - 🥇

		0, 10, 10,	00.1001		. U. UUL 1	0.100	
The successful set is	38	903940	80.193	1.009	18.102	0.695	
<ul> <li>The workbook</li> </ul>	39	932948	80.203	1.016	18.076	0.705	
contains a	40	961778	80.065	1.018	18.221	0.696	
worksheet for	41	990701	80.181	1.015	18.091	0.714	
each gas	42	1019570	80.185	1.031	18.077	0.707	
stream.	43	1048680	80.149	1.023	18.125	0.704	
Stroutil.	44	1077430	80.12	1.023	18.155	0.702	
	45	1106301	80.076	1.013	18.218	0.693	
Data for up to 80 gas	46	1135051	80.207	0.996	18.099	0.698	
sample streams	47	1163923	80.185	1.018	18.089	0.708	
-	48	1192796	80.148	0.997	18.172	0.684	
	49	1221002	, 80 195	1 011	18.1	<u></u>	
	ļN - N	► ► ► Strea	am 1 / Stream 3	/ Stream 4	/ Stream 5 /	Stream 7 /	
	Read	ły					

200-07	
25E-07	
24E-07	
24E-07	
24E-07	
2.4E 07	



### **OPC – Data Output**

The screen shot is from an OPC data viewer showing data tags for each stream and for each gas channel.

RQ/CER/OUR data can be output for each stream

	OPC data	can be	selected	as raw,	corrected	or %, PPIVI	values	
atrikonO	PC Explorer - [Untitled*]							
Server	Group Item View Help							

ODC data and he calested as your as we stad as 0/ DDM values

MatrikonOPC Explorer - [Untitled*]					
File Server Group Item View Help					
£ ★ 🗊 🖄   🗳 ❹ 孜 ⑭   Ø ອ   💩 🚳 🔉 🍁 🖄					
1	Contents of '1'				
E	Item ID	Access Path Value	Quality	Timestamp	Status
GT Matrikon.OPC.Simulation.1	1. \QGAPro\2_1	79.1131058460503	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
E- I National Instruments. Variable Engine. 1	10 \\. \QGAPro\2_10	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
Land 1	1. \QGAPro\2_11	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
Machine Is Not Browsed	1. \QGAPro\2_12	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
Other Network Computers	10 \\. \QGAPro\2_13	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	100 \\. \QGAPro\2_14	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	100 \\. \QGAPro\2_15	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	(\. \QGAPro \2_16 \. \QGAPro \2_2	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	(), (QGAPro \2_2 (), \QGAPro \2_3	18.7962157343888 0.8728409069347	Good, non-specific Good, non-specific	11/29/2011 9:10:42.444 AM 11/29/2011 9:10:42.444 AM	Active Active
Tage are automatically	(), \QGAPro\2_5	4557.52377693532	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
Tags are automatically	(), (QGAPro \2_5	1.21783751262622	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	1, \QGAPro\2_6	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
updated for the active streams:	1. \QGAPro \2 7	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	10 \\. \QGAPro \2_8	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
$\lambda O \subset A D = \lambda O $	1. \QGAPro\2_9	0	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
\\OGAPro\2 2 is the current value for	W \\. \QGAPro\2_CER	0.00121341998855826	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
	W \\. \QGAPro\2_OUR	0.00184848166579476	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
stroom 2 gos 2	W \\. \QGAPro\2_RQ	0.656441451928897	Good, non-specific	11/29/2011 9:10:42.444 AM	Active
stream 2 gas 2.	1. \QGAPro\3_1	79.3545815798548	Bad, non-specific	11/28/2011 2:00:14.542 PM	Active
	10 \\. \QGAPro\3_10	0	Bad, non-specific	11/28/2011 2:00:14.543 PM	Active
\\QGAPro\2_RQ is the current	11 \\. \QGAPro\3_11	0	Bad, non-specific	11/28/2011 2:00:14.544 PM	Active
	100 \\. \QGAPro \3_12	0	Bad, non-specific	11/28/2011 2:00:14.544 PM	Active
DO value for stream 2	(\.\QGAPro\3_13)	0	Bad, non-specific	11/28/2011 2:00:14.544 PM 11/28/2011 2:00:14.544 PM	Active
RQ value for stream 2.	(), (QGAPro\3_14	0	Bad, non-specific Bad, non-specific	11/28/2011 2:00:14.544 PM 11/28/2011 2:00:14.544 PM	Active Active
	(), \QGAPro\3_16	0	Bad, non-specific Bad, non-specific	11/28/2011 2:00:14.545 PM	Active
	(), \QGAPro\3_2	1.51106640662871	Bad, non-specific	11/28/2011 2:00:14.542 PM	Active
	1. \QGAPro\3_3	18,437938745529	Bad, non-specific	11/28/2011 2:00:14.542 PM	Active
	100 \\. \QGAPro\3 4	0.696413267987495	Bad, non-specific	11/28/2011 2:00:14.542 PM	Active
	100 \\. \QGAPro\3_5	0	Bad, non-specific	11/28/2011 2:00:14.543 PM	Active

info@hiden.co.uk



### Real-time data export, system control and I/O for process control

#### Three options for output of real time data

- OPC for process control providing real time data tags from QGA Pro software.
- RS232 streamed data in ascii format from the mass spectrometer interface unit.
- Socket interface for windows client compatible applications with MASsoft Pro software.

#### System control and outputs

- 5 I/O for TTL signal control for automatic operation- start /stop for example.
- Up to 16 channel signal output options -0-10V analogue outputs.

#### System data logging

- Three RS485 inputs provide for up to three device type protocols for reading data from external devices, temperature for example. Synchronously logged and displayed with the mass spectrometer data.
- Up to 16 channel signal output options as 0-10V analogue.



# QIC BioStream gas analyser for sampling fermentors with sample flow rates in the range of litres /min to 0.1 l/min

- Small diameter sample tubing is used to connect the QIC BioStream to the fermentors.
- Sample gas flow through the sample tubing is induced by creating a pressure gradient along the tube.
- The sample flow may be achieved by running the fermentor at a positive pressure & venting the sample flow to ambient pressure after analysis.
- Alternatively, a sampling pump may be connected to the analyzer exhaust.
- This type of system will typically accept individual sample flow rates from several litres/minute to 0.1 litres/minute. Sample transit times become unacceptably long (several minutes) below 0.02 litres/minute.
- Small fermentors and miniature reactors use the low flow configuration with flow rate < 4ml/minute.



# QIC BioStream gas analyser for small fermentors with very low flow 4ml/min

- The QIC BioStream low flow system utilizes the unique capability of the Proteus multistream selector valve to operate under very low pressure (vacuum) conditions.
- This system is optimized for fast response with very low sample flow rates. This is achieved with small-bore capillary tubing. The sampling lines then become the 1st stage of the inlet pressure reduction system. The exhaust of the Proteus valve is connected to the dry scroll pump to provide a vacuum of a few mbars absolute within the valve.
- Atmospheric pressure sample gas enters the capillary sample tubing at the sampling point at 1.8 metres/sec (typical for 0.2mm ID x 2.0 metre sampling capillary) then accelerates rapidly along the tubing due to the progressive expansion of the sample.
- For example, 4 ml/minute atmospheric flow expands to 4 x >200 = 800 ml/min (0.8 litres/minute
- This increase in sample volume flow rate provides rapid sample transit along the sampling capillary & the fast switching response, switching time between sample streams is < 0.6 seconds.</li>



# **Connecting to fermentors with low flow**

20, 40 or 80 way systems are available in low flow configuration.



Low flow 40 way Proteus multistream sampling valve Configuration. The Proteus multi stream valve is close coupled to the mass spectrometer vacuum for low flow.



Sampling lines for low flow sampling , female luer lock fittings, shown with disposable hydrophobic filters< operates with flow ~ 4ml/min.



# Sample conditioning for the analyser

The QIC BioStream off gas analyser requires sample to be:

#### Non condensing.

A hydrophobic filter should be included in each sample line to avoid water droplets entering the analyser.

#### and without any foam or overspill.

For larger reactors a simple foam trap in the sample line avoids liquid entering the analyser.

For advice on how to connect fermenters to Hiden's QIC BioStream real time gas analyser- please send a schematic detailing your fermenter layout, flow rates, and gas/vapour species.



# Summary – QIC BioStream for off-gas analysis

QIC BioStream – cart or compact bench top configuration

Off gas analysis for 8, 20, 40, or 80 streams

Analysis of gases and vapours

Triple filter quadrupole mass spectrometer

OUR/CER/RQ

Data output though OPC shared variable engine

#### Lifetime application and service support




QIC BioStream mobile cart



QIC BioStream-C bench top

- <u>www.HidenAnalytical.com</u>
- The Hiden website is an excellent resource with product pages, brochures, catalogues, product pages with some application notes, presentation and other information.
- Contact +44 1925 445225 for direct support.



A MANARA